

Fig.1

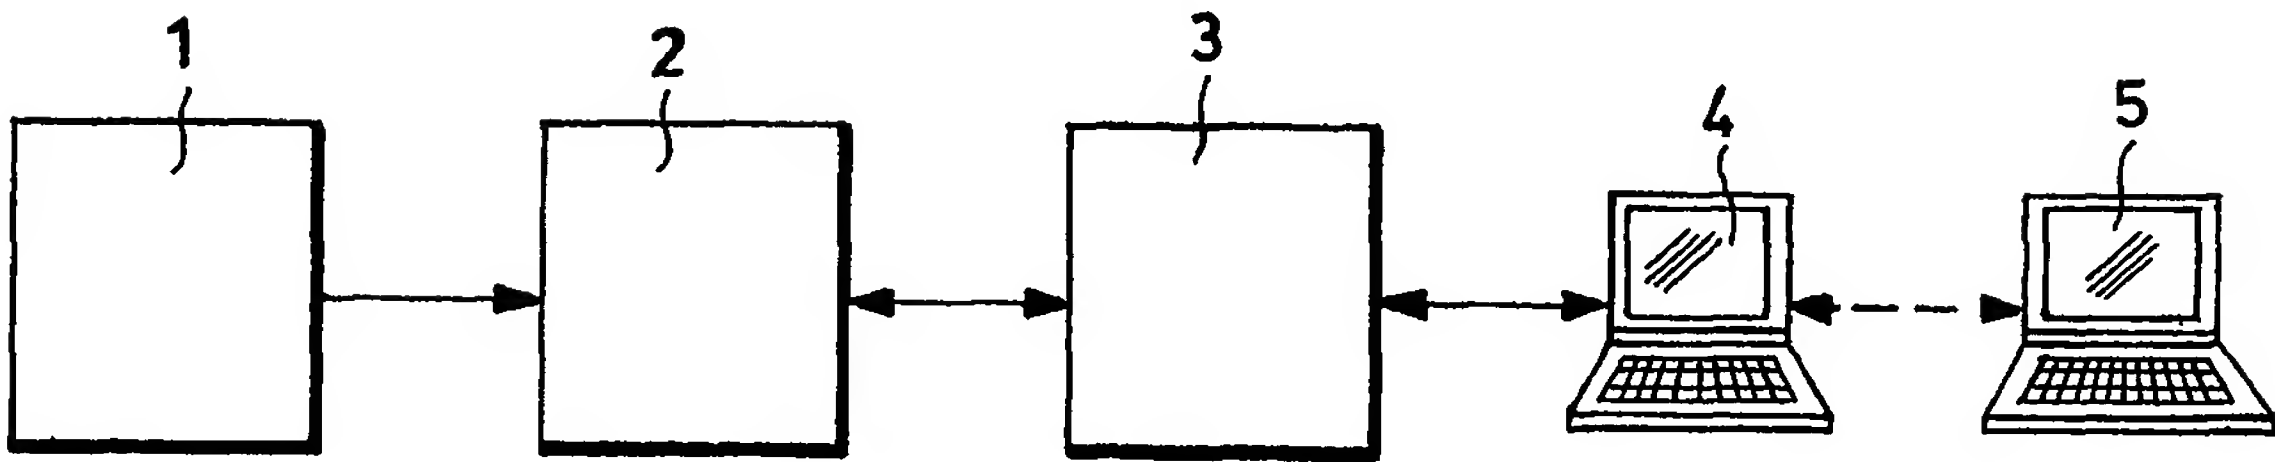
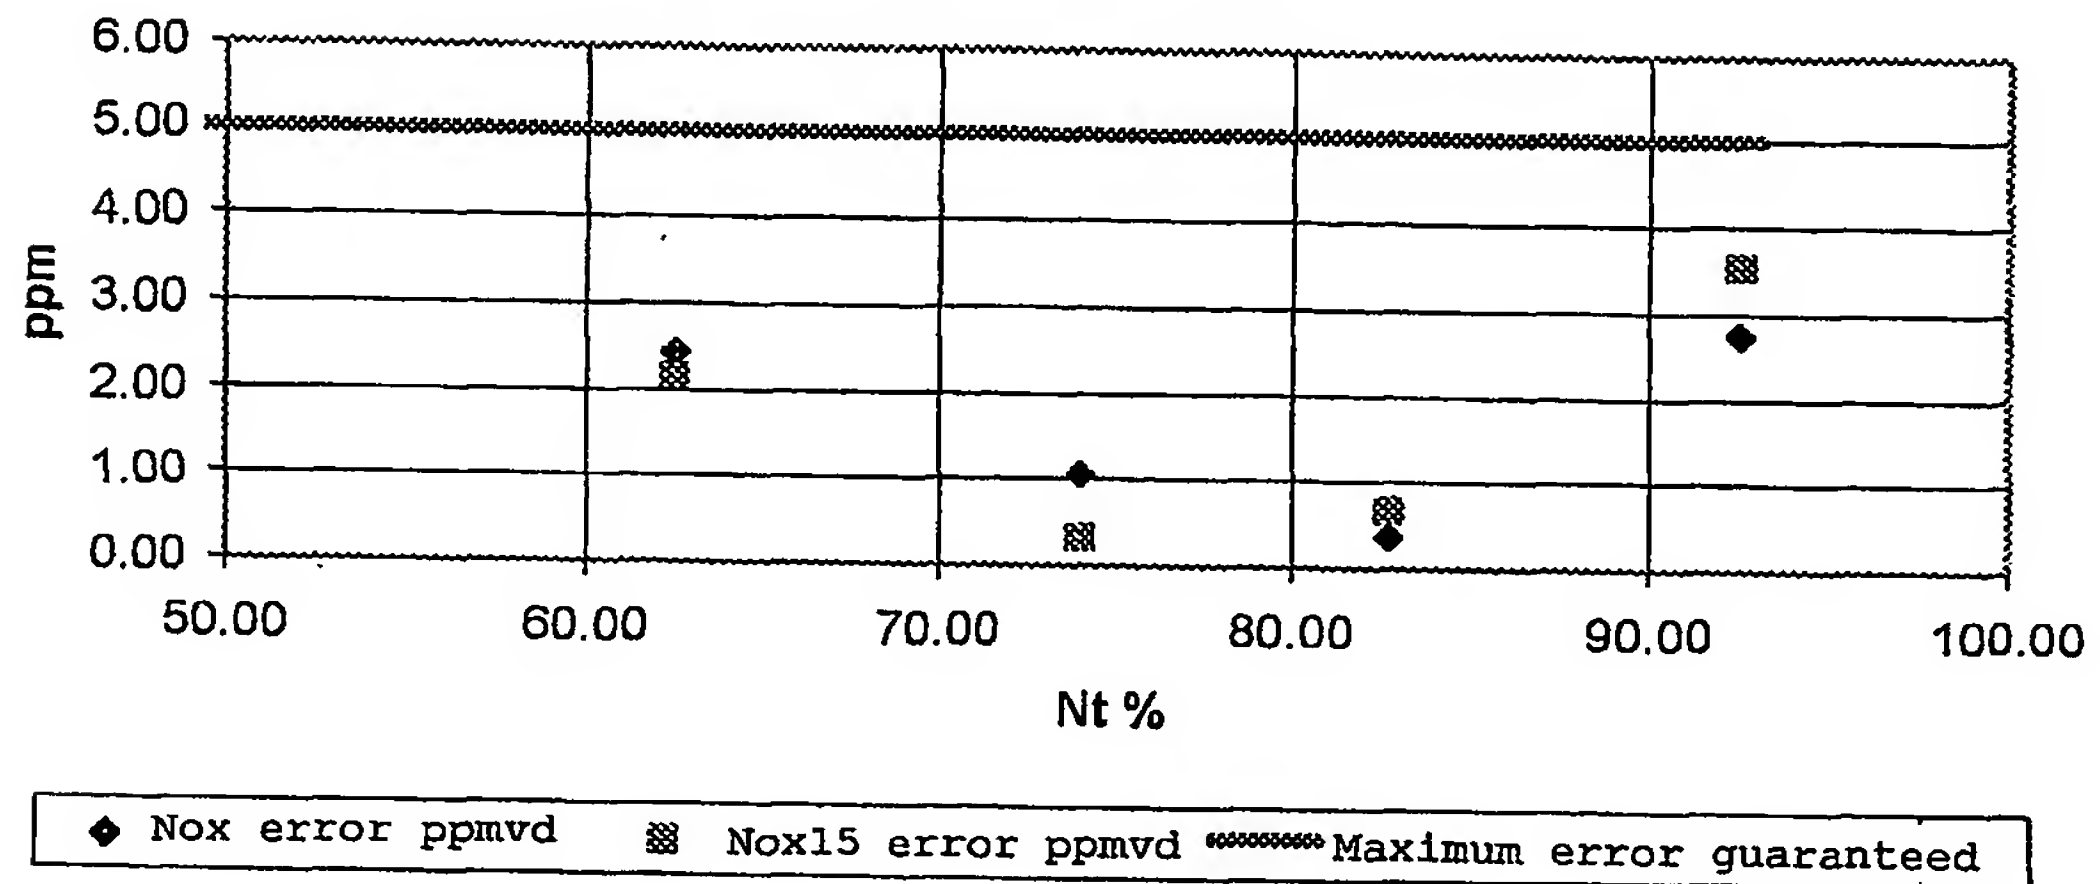


Fig.2

2/3


Nox error estimation

Unit: GE10 B2 DLN

Fig.3a

CO error estimation

Unit: GE10 B2 DLN

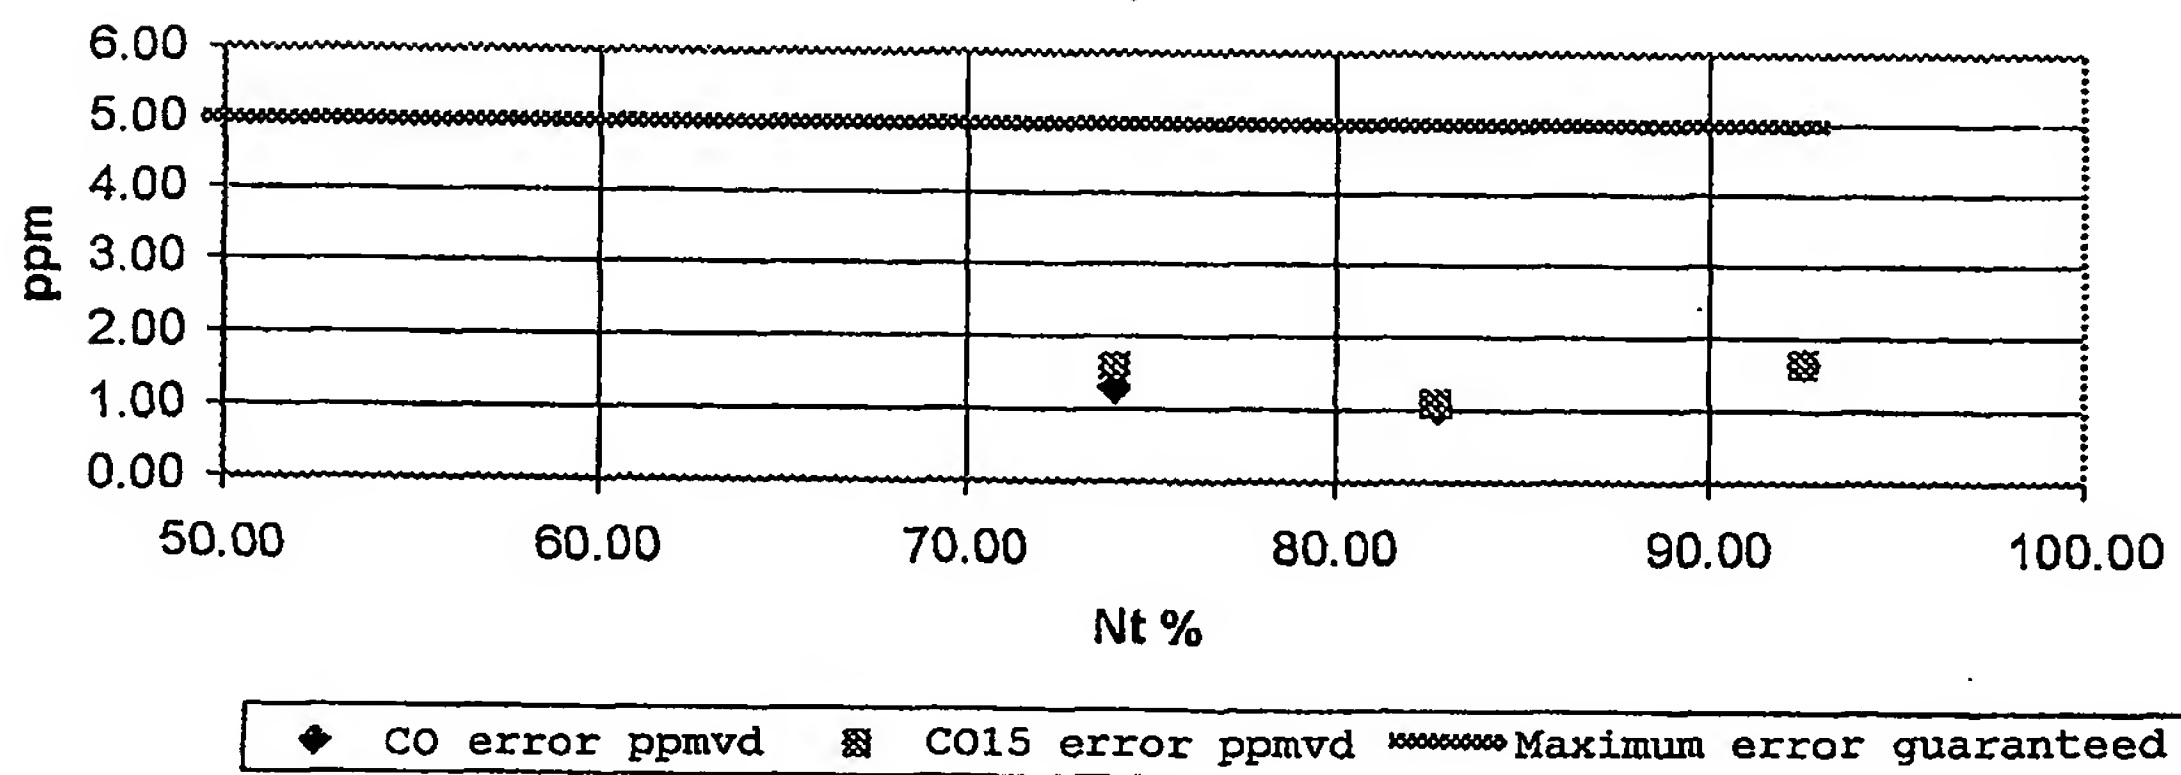Fig.3b

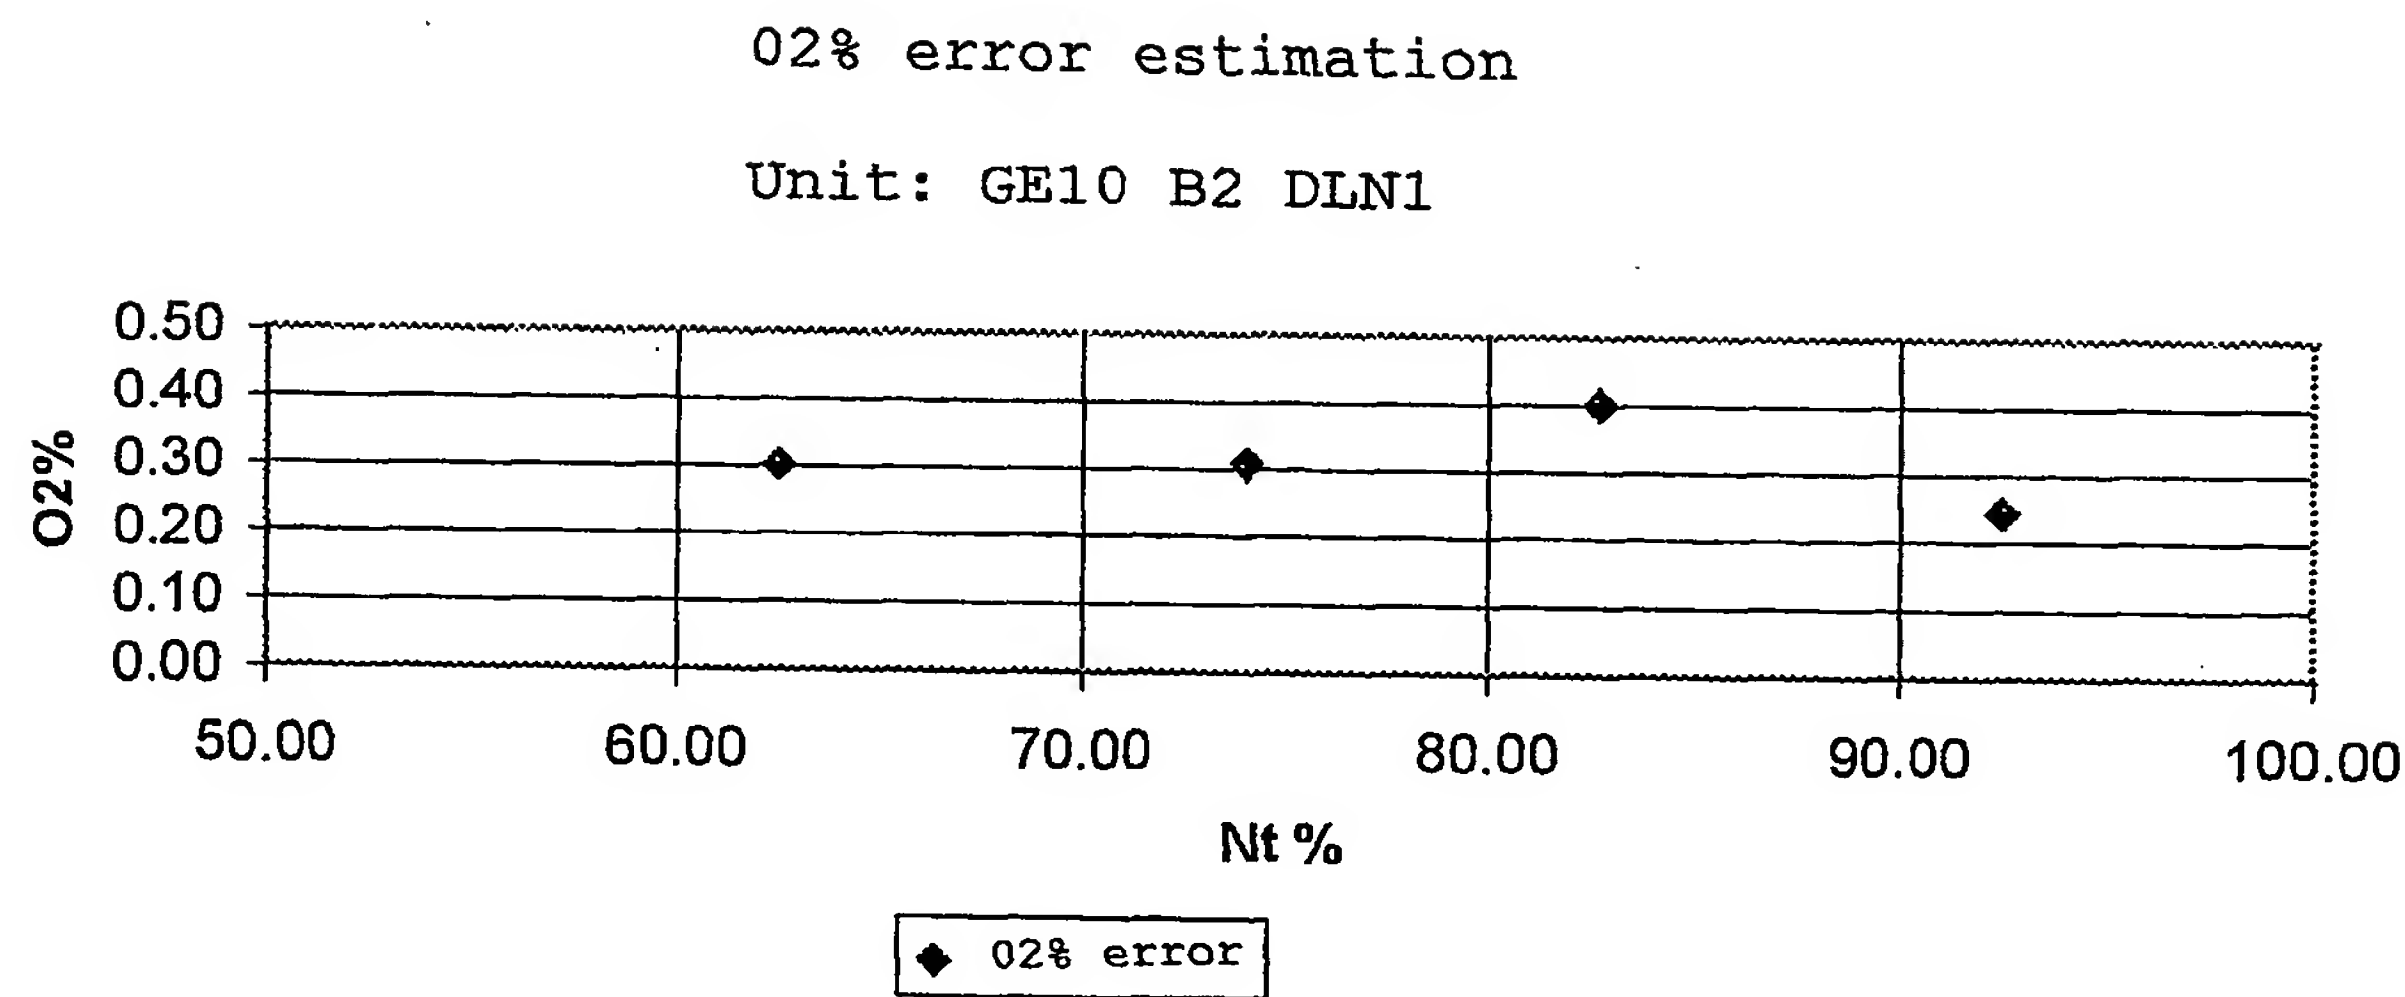


Fig.3c